# CleanMount **Quick Start Installation Guide**

### What's Included

- A) 1/4" Hex Key B) (4) Display Thumb Screws (M4 x 8)
- C) (4) Display Thumb Screws (M4 x 12)

D) Rail cover

### **Tools You'll Need**


#### • #1 Phillips screwdriver

• Wire Cutter & Tie Wraps (for securing keyboard and mouse cabling: see Step 5 for instructions on accessing prewired USB hub)



#### 1. Install Mounting Track\*


\* Refer to track installation instructions

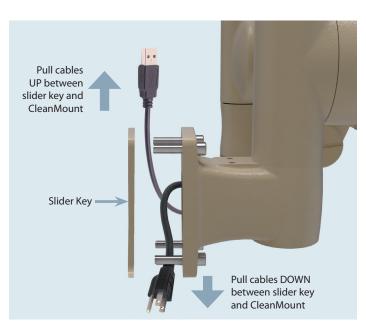

### 2. Orient Cables


1. Remove track slider key

2. Orient cables in the proper direction (up or down) and reattach slider key to CleanMount base

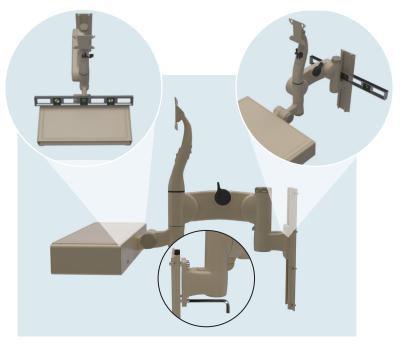


#### 4. Level and Tighten

Use 1/4" Hex Key to Tighten Four Slider Key Bolts

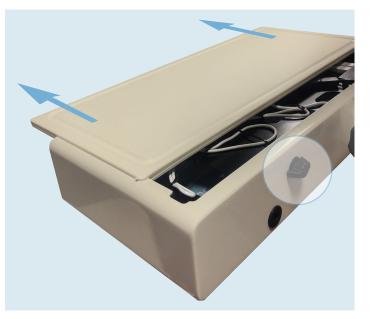

#### **5. USB Hub Access**

1) Turn latch on rear of keyboard enclosure to release cover. Pull cover forward to access the USB hub.

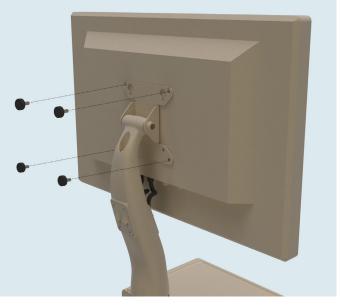


### 6. Install Display

Using (4) M4 x 8 Display Thumb Screws, attach display to CleanMount. (NOTE: If the M4 x 8 Display Thumb Screws can't be threaded sufficiently to provide a secure attachment, use the M4 x 12 Display Thumb Screws instead.)




## **STRONGARM**healthcare

Visit strongarmhealthcare.com to view our installation video.

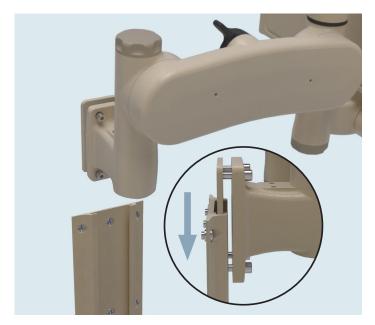

#### 3. Install Onto Track

(Shown here without cabling)

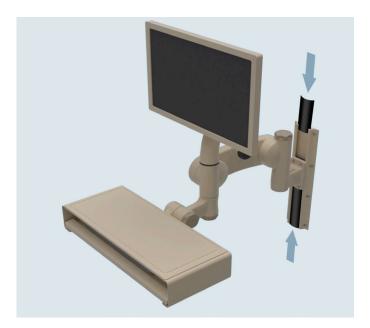


#### 7. Install Track Cable Cover


Cut supplied rail cover to desired length(s) and slide into track channels as shown

# CleanMount **Operation Guide**


Visit strongarmhealthcare.com to view our complete operations video.

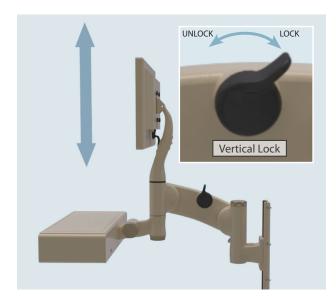


**Vertical Adjustment** 

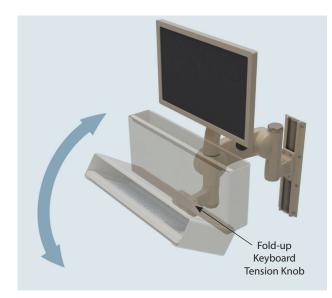


Fold-up Keyboard

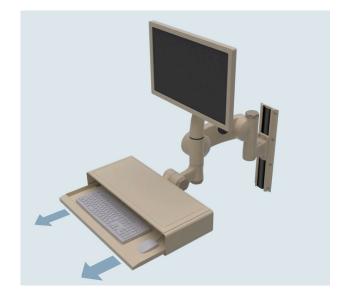

**Pullout Keyboard Tray** 

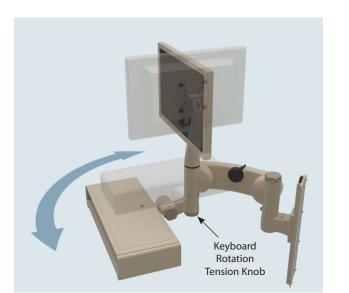

**Keyboard Rotation** 

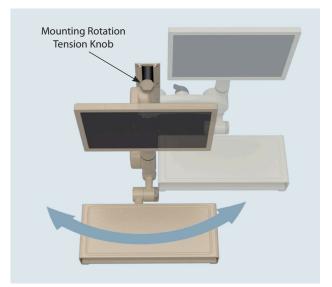


**Mounting Rotation** 




Slide Out Mouse Tray (optional)

## **STRONGARM**healthcare

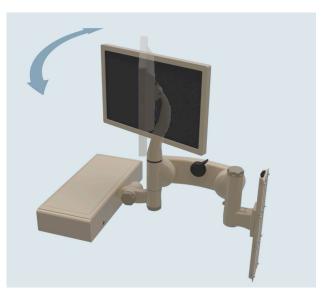

#### PatientView\* Display Rotation

(\*On PatientView equipped models)

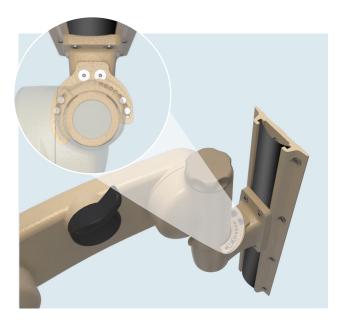

Rotational Stop (optional\*)

(\*See instructions included with Rotational Stop for installation and operation guide)